

इंटरनेट

मानक

### Disclosure to Promote the Right To Information

Whereas the Parliament of India has set out to provide a practical regime of right to information for citizens to secure access to information under the control of public authorities, in order to promote transparency and accountability in the working of every public authority, and whereas the attached publication of the Bureau of Indian Standards is of particular interest to the public, particularly disadvantaged communities and those engaged in the pursuit of education and knowledge, the attached public safety standard is made available to promote the timely dissemination of this information in an accurate manner to the public.

“जानने का अधिकार, जीने का अधिकार”

Mazdoor Kisan Shakti Sangathan

“The Right to Information, The Right to Live”

“पुराने को छोड़ नये के तरफ”

Jawaharlal Nehru

“Step Out From the Old to the New”

IS 2720-39-2 (1979): Methods of test for soils, Part 39: Direct shear test for soils containing gravel, Section 2: In-situ shear test [CED 43: Soil and Foundation Engineering]



“ज्ञान से एक नये भारत का निर्माण”

Satyanarayan Gangaram Pitroda

“Invent a New India Using Knowledge”



“ज्ञान एक ऐसा खजाना है जो कभी चुराया नहीं जा सकता है”

Bhartrhari—Nitiśatakam

“Knowledge is such a treasure which cannot be stolen”



BLANK PAGE



*Indian Standard*

**METHODS OF TEST FOR SOILS  
PART XXXIX DIRECT SHEAR TEST FOR SOILS  
CONTAINING GRAVEL**

**Section 2 *In-Situ* Shear Test**

( First Reprint NOVEMBER 1988 )

UDC 624.131.377:624.131.212

© Copyright 1979

**BUREAU OF INDIAN STANDARDS  
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG  
NEW DELHI 110002**

*Indian Standard*

## METHODS OF TEST FOR SOILS

PART XXXIX DIRECT SHEAR TEST FOR SOILS  
CONTAINING GRAVELSection 2 *In-Situ* Shear Test

Soil Engineering and Rock Mechanics Sectional Committee, BDC 23

*Chairman*

PROF DINESH MOHAN

*Representing*Central Building Research Institute ( CSIR ),  
Roorkee*Members*

ADDITIONAL DIRECTOR RESEARCH, ( FE ), RDSO	Railway Board ( Ministry of Railways )
DEPUTY DIRECTOR RESEARCH, ( FE-I ), RDSO ( <i>Alternate</i> )	
PROF ALAM SINGH	University of Jodhpur, Jodhpur
LT-COL AVTAR SINGH	Engineer-in-Chief's Branch, Army Headquarters
MAJ V. K. KANITKAR ( <i>Alternate</i> )	
DR A. BANERJEE	Cementation Co Ltd, Calcutta
SHRI S. GUPTA ( <i>Alternate</i> )	
DR R. K. BHANDARI	Central Building Research Institute ( CSIR ), Roorkee
CHIEF ENGINEER ( D&R )	Irrigation Department, Government of Punjab, Chandigarh
DIRECTOR ( IPRI ) ( <i>Alternate</i> )	
SHRI K. N. DADINA	In personal capacity ( P-20 New Alipore, Calcutta 700053 )
SHRI A. G. DASTIDAR	In personal capacity ( 5 Hungerford Street, 12/1 Hungerford Court, Calcutta 700017 )
DR G. S. DHILLON	Indian Geotechnical Society, New Delhi
DIRECTOR ( CSMRS )	Central Water Commission, New Delhi
DEPUTY DIRECTOR ( CSMRS ) ( <i>Alternate</i> )	
SHRI A. H. DIVANJI	Asia Foundations & Construction ( P ) Ltd, Bombay
SHRI A. N. JANGLE ( <i>Alternate</i> )	
DR GOPAL RANJAN	University of Roorkee, Roorkee; and Institution of Engineers ( India ), Delhi Centre

( *Continued on page 2* )

© Copyright 1979

## BUREAU OF INDIAN STANDARDS

This publication is protected under the *Indian Copyright Act* ( XIV of 1957 ) and reproduction in whole or in part by any means except with written permission of the publisher shall be deemed to be an infringement of copyright under the said Act.

( Continued from page 1 )

<i>Members</i>	<i>Representing</i>
DR SHASHI K. GULHATI	Indian Institute of Technology, New Delhi
DR G. V. RAO ( <i>Alternate</i> )	
SHRI O. P. MALHOTRA	Public Works Department, Government of Punjab, Chandigarh
SHRI T. K. NATARAJAN	Central Road Research Institute ( CSIR ), New Delhi
REPRESENTATIVE RESEARCH OFFICER	Irrigation Research Institute, Khagaul, Patna
SHRI K. R. SAXENA	Building & Roads Research Laboratory, Chandigarh
SECRETARY	Engineering Research Laboratories, Hyderabad
DEPUTY SECRETARY ( <i>Alternate</i> )	Central Board of Irrigation & Power, New Delhi
SHRI M. M. D. SETH	Public Works Department, Government of Uttar Pradesh, Lucknow
DR B. L. DHAWAN ( <i>Alternate</i> )	
SHRI M. K. SINGHAL	Irrigation Research Institute, Roorkee
SHRI N. SIVAGURU	Roads Wing ( Ministry of Shipping & Transport )
SHRI D. V. SIKKA ( <i>Alternate</i> )	
SHRI K. S. SRINIVASAN	National Buildings Organization, New Delhi
SHRI SUNIL BERRY ( <i>Alternate</i> )	
SUPERINTENDING ENGINEER ( P&D )	Public Works Department, Government of Tamil Nadu, Madras
EXECUTIVE ENGINEER ( SM&RD ) ( <i>Alternate</i> )	
SHRI B. T. UNWALLA	Concrete Association of India, Bombay
SHRI T. M. MENON ( <i>Alternate</i> )	
SHRI H. C. VERMA	All India Instruments Manufacturers & Dealers Association, Bombay
SHRI V. S. VASUDEVAN ( <i>Alternate</i> )	
SHRI D. AJITHA SIMHA, Director ( Civ Engg )	Director General, BIS ( <i>Ex-officio Member</i> )

*Secretary*

SHRI K. M. MATHUR  
Deputy Director ( Civ Engg ), BIS

Soil Testing Procedures and Equipment Subcommittee, BDC 23 : 3

*Convener*

PROF ALAM SINGH                      University of Jodhpur, Jodhpur

*Members*

SHRI AMAR SINGH                      Central Building Research Institute ( CSIR ),  
Roorkee

SHRI N. M. PATEL ( *Alternate* )  
LT-COL AVTAR SINGH                      Engineer-in-Chief's Branch, Army Headquarters  
MAJ V. K. KANITKAR ( *Alternate* )

( Continued on page 12 )

# *Indian Standard*

## METHODS OF TEST FOR SOILS

### PART XXXIX DIRECT SHEAR TEST FOR SOILS CONTAINING GRAVEL

#### Section 2 *In-Situ* Shear Test

## 0. FOREWORD

**0.1** This Indian Standard ( Part XXXIX/Sec 2 ) was adopted by the Indian Standards Institution on 11 July 1979, after the draft finalized by the Soil Engineering and Rock Mechanics Sectional Committee had been approved by the Civil Engineering Division Council.

**0.2** With a view to establishing uniform procedures for the determination of different characteristics of soils and also for facilitating a comparative study of the results, the Indian Standards Institution is bringing out this Indian Standard on methods of test for soils ( IS : 2720 ) which is being published in parts. Fortyone parts of this standard have been published so far. This part covers direct shear test. The test is of two kinds depending upon the state of samples, namely, laboratory test and *in-situ* test. The laboratory test is covered in Section 1 of this part. This part [ IS : 2720 ( Part XXXIX/Sec 2 )-1979 ] deals with *in-situ* determination by direct shear, the shear strength of soils containing gravel and cobblestone.

**0.3** In the formulation of this standard due weightage has been given to international co-ordination among the standards and practices prevailing in different countries in addition to relating it to the practices in the field in this country.

**0.4** In reporting the result of a test or analysis made in accordance with this standard, if the final value, observed or calculated, is to be rounded off, it shall be done in accordance with IS : 2-1960\*.

---

## 1. SCOPE

**1.1** This standard ( Part XXXIX/Sec 2 ) covers the method for the determination by direct shear, the *in-situ* shear strength of soils containing gravels and cobblestone.

---

\*Rules for rounding off numerical values ( revised ).

## 2. APPARATUS

**2.1 Shear Box** — The side of the shear box shall be not less than 10 times the maximum expected particle size and the thickness of the samples not less than three times the maximum particle size. For convenience in handling the box could be of built-up sections from plates. The four sides of the box could be connected through bolts and nuts designed properly to form the box. Figure 1 shows the suggested size with 1 500 × 1 500 mm sample size.

**2.2 Top Loading Plate ( see Fig. 2 )** — A rigid steel plate fitting in the shear box suitably designed to distribute the load uniformly over the sample normal to the shear plane.

**2.3 Hydraulic Jack** — Suitable remote control hydraulic jack of adequate capacity for applying shear force.

**2.4 Rolled Steel Joist and Wooden Sleepers** — Adequate number of rolled steel joist and wooden sleepers and sand bags for making a platform and providing adequate kentledge for applying normal load on the sample.

**2.5 Rollers** — Suitable size of rollers equal to the width of plates forming the shear box frame to be placed in between the side of the box and a bed plate on either side of the box.


**2.6 Datum Bars** — Suitable section of steel bars to be hinged for two pegs fixed at a distance equal to the side of the box driven to a depth of minimum 500 mm on either side of the box.

**2.7 Spring Balance** — Spring balance of 10 kg capacity of sensitivity 1'0 kg to weigh the sand bags.

## 3. PREPARATION OF SPECIMEN


**3.1** A steel box made out of mild steel plates of adequate thickness, provided with a cutting edge with the required internal dimension may be used for trimming the sample. This hollow box be pressed into the deposit under a load applied by hydraulic jack ( see Fig. 3 ). The soil around the box be excavated, simultaneously with the penetration of the box to facilitate its easy sinking. Care shall be taken to ensure that the box shall sink in vertical position.

**3.1.1** Alternatively, during excavation two blocks, of the required size be left undisturbed at the desired position. After the excavation is completed the assembled boxes shall be put on the top of the block and soil below the plate shall be excavated gradually till the boxes reach the required position.

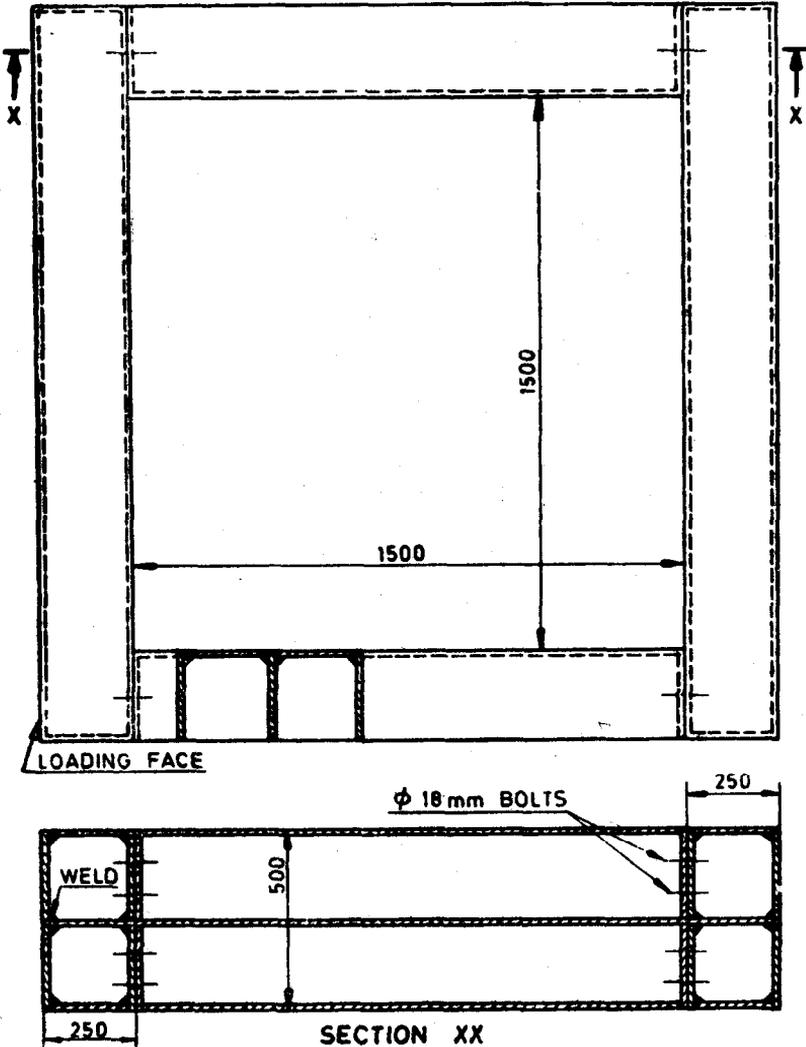

NOTE — All members fabricated out of 10 mm thick plates.  
All dimensions in millimetres.

FIG. 1 SHEAR BOX 1 500 × 1 500 mm SIZE

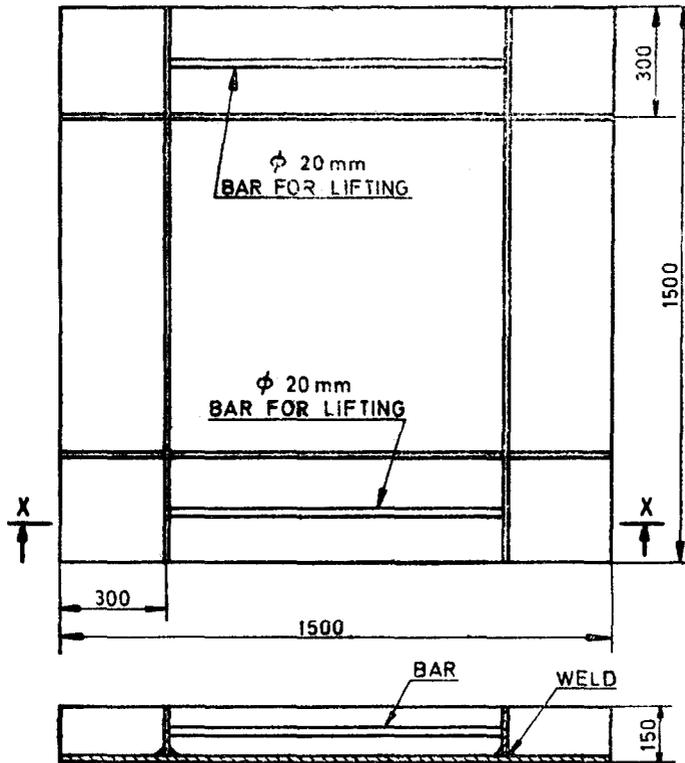

SECTION XX

NOTE—All members fabricated out of 10 mm thick plates.  
All dimensions in millimetres.

FIG. 2 TOP LOADING PLATE

3.2 Two rolled steel joists form the bed plates. A train of rollers shall be put in between the sides of the box and the bed plates on either side of the box. Gravels projecting above box frames shall be removed and the gap shall be filled up with medium to fine sand to give level surface for better seating of the top plate.

3.3 The loading cap befitting the internal dimension of the box made of steel plates of adequate thickness be placed on the soil.

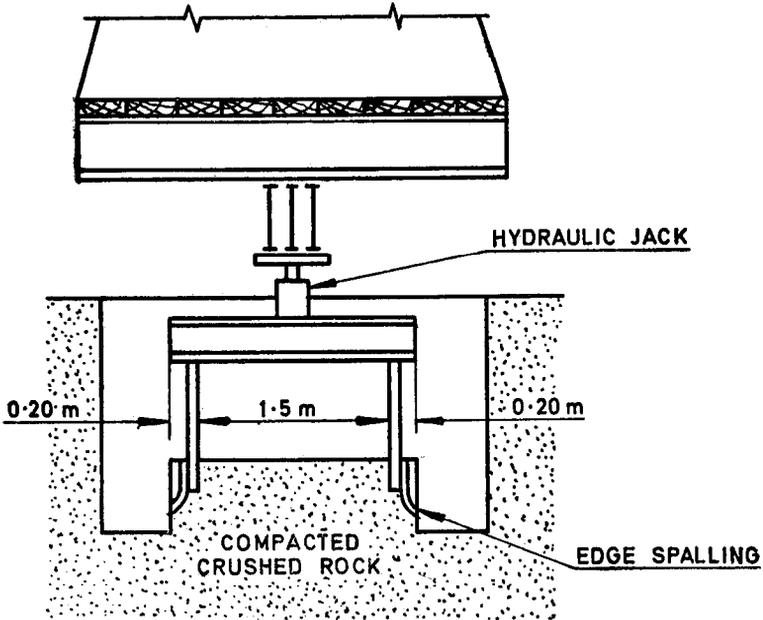


FIG. 3 ARRANGEMENT FOR OBTAINING SPECIMEN  
FOR *In-Situ* SHEAR TEST

**3.4** The test should be carried out at moisture content as close to field condition as possible.

NOTE — In case of soils containing fines more than 12 percent, the test may be conducted in soaked state to simulate for worst field conditions; the soaking period may extend up to 4 days depending upon type of soils.

#### 4. APPLICATION OF NORMAL LOAD

**4.1** The normal load on the sample shall be applied with the help of a platform made of rolled steel joist and wooden sleepers and loaded with sand bags ( see Fig. 4 ).

#### 5. TEST PROCEDURE

**5.1** The shear force shall be applied through a remote control hydraulic jack and proving ring arrangement taking reaction from the adjacent box ( see Fig. 4 ).

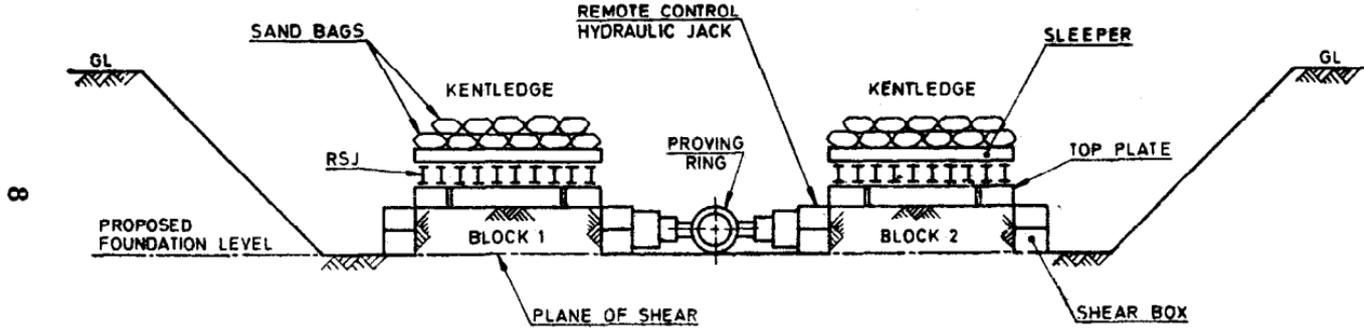


FIG. 4 TEST SET UP FOR LARGE SIZE *In-Situ* SHEAR TEST

**5.2** Two tests at different normal pressures shall be carried out at one location. After the block with lesser normal pressure failed, the space between the failed block and the side of the pit shall be blocked by boulders and also by struting. The normal load on failed block shall be increased, and then the test on the other block shall be completed by taking reaction of shear force from the failed block.

**5.3** The jack shall be so fitted so that the application of the lateral load occurs as far as possible near to the plane of shear.

**5.4** The test shall be conducted by giving an equal increment of shear load under the normal load, each increment of shear load shall be maintained constant till the equilibrium conditions are reached, the readings shall be recorded with the help of suitably mounted dial gauges. The next increment of shear load shall then be applied and the process continued till the failure of the specimen occurs. The normal loads applied shall be more than the existing over-burden and cover the anticipated loading range in the area. The range of normal load should represent the site loading conditions as far as possible. Two more tests at different normal loads shall be carried out at adjacent location, to make four tests, a minimum number required necessary for interpretation.

## **6. CALCULATION AND REPORT**

**6.1** Results of test shall be recorded suitably. A recommended pro forma for recording the results is given in Appendix A.

**6.2** The horizontal displacement at a particular load shall be recorded from shear displacement dial readings.

**6.3** The maximum shear force shall be peak load from load displacement curve or where the tangent of flatter portion of the later part of the curve leaves in case the curve does not give peak point.

**6.4** The maximum shear stress and the corresponding horizontal displacement and applied normal stress shall be recorded for each test and the result be presented in the form of a graph in which the applied normal stress is plotted as abscissa and shear stress as ordinate. The angle which the resulting straight line makes with the horizontal axis and the intercept which the straight line makes with the vertical axis shall be reported as the angle of shearing resistance and cohesion respectively.

**NOTE** — The normal stress versus maximum shear stress relationship may not be straight line in all cases. In such cases the shear parameter shall be obtained by drawing tangent to the normal stress and maximum shear stress curve at the point of normal stress expected in the field.

**A P P E N D I X   A**

( Clause 6.1 )

**I   P R O   F O R M A   F O R   R E C O R D I N G   I N - S I T U   T E S T   R E S U L T S**

Project .....      Location of sample .....

Rate of load .....      Specimen No. ....  
  increment .....      Depth of test .....

                                 Proving ring No. ....

                                 Providing ring constant .....

                                 Normal load applied .....

**S O I L   S P E C I M E N   M E A S U R E M E N T**

Dimensions .....      Maximum size of particle .....

Initial water content .....      Area of specimen .....

Final water content .....      Height of specimen .....

                                 Volume of specimen .....

                                 Unit weight of soil .....

**II   P R O   F O R M A   F O R   R E C O R D I N G   S H E A R I N G   S T A G E**

- i) Thickness of sample ..... mm
- ii) Area of cross section of sample ..... cm<sup>2</sup>
- iii) Rate of shearing ..... mm/min
- iv) Normal stress applied ..... kg/cm<sup>2</sup>

Date & Time	Shear Displacement Dial Reading	Shear Displacement	Average Shear Displacement	Proving Ring Reading	Shear Force	Shear Stress	Vertical Reading	Vertical Displacement
	$D_{hs}$ $D_{hs}$	$D_{hs}$ $D_{hs}$					$D_{rs}$ $D_{rs}$	$D_{rs}$ $D_{rs}$

Average Vertical Displacement

Plot — Shear stress versus shear displacement and find:  
 a) maximum shear stress at the peak of curve, and  
 b) corresponding shear displacement.

### III PRO FORMA FOR RECORDING SUMMARY OF RESULTS

Test No.	Normal Stress	Proving Ring Constant	Shear Stress at Failure	Shear Displacement at Failure	Initial Water Content	Final Water Content	Remarks
----------	---------------	-----------------------	-------------------------	-------------------------------	-----------------------	---------------------	---------

Plot — Shear stress-normal stress relationship to obtain:  
 a) cohesion intercept, and  
 b) angle of shearing resistance.

**IS : 2720 ( Part XXXIX/Sec 2 ) - 1979**

( Continued from page 2 )

<i>Members</i>	<i>Representing</i>
DEPUTY DIRECTOR RESEARCH ( FE-II ) ( RDSO )	Ministry of Railways
DEPUTY DIRECTOR RESEARCH ( SM-III ) ( RDSO ) ( <i>Alternate</i> )	
DIRECTOR ( CSMRS )	Central Water Commission, New Delhi
DEPUTY DIRECTOR ( CSMRS ) ( <i>Alternate</i> )	
DR GOPAL RANJAN	University of Roorkee, Roorkee
SHRI H. K. GUHA	Geologists Syndicate Pvt Ltd, Calcutta
SHRI N. N. BHATTACHARAYA ( <i>Alternate</i> )	
SHRI SHASHI K. GULHATI	Indian Institute of Technology, New Delhi
SHRI O. P. MALHOTRA	Public Works Department, Government of Punjab, Chandigarh
RESEARCH OFFICER ( <i>Alternate</i> )	
SHRI P. JAGANNATHA RAO	Central Road Research Institute ( CSIR ), New Delhi
REPRESENTATIVE	Irrigation Research Institute, Khagaul, Patna
SHRI M. M. D. SETH	Public Works Department, Government of Uttar Pradesh, Lucknow
DR B. L. DHAWAN ( <i>Alternate</i> )	
SHRI H. C. VERMA	Associated Instruments Manufacturers ( I ) Pvt Ltd, New Delhi
PROF T. S. NAGARAJ ( <i>Alternate</i> )	

# BUREAU OF INDIAN STANDARDS

## Headquarters :

Manak Bhavan, 9 Bahadur Shah Zafar Marg, NEW DELHI 110002

Telephones : 3 31 01 31, 3 31 13 75

Telegrams : Manaksanstha  
( Common to all Offices )

## Regional Offices :

Telephone

\*Western ; Manakalaya, E9 MIDC, Marol, Andheri ( East ), 6 32 92 95  
BOMBAY 400093

†Eastern : 1/14 C I. T. Scheme VII M, V. I. P. Road, 36 24 99  
Maniktola, CALCUTTA 700054

Northern : SCO 445-446, Sector 35-C { 2 18 43  
CHANDIGARH 160036 { 3 16 41

Southern : C. I. T. Campus, MADRAS 600113 { 41 24 42  
{ 41 25 19  
{ 41 29 16

## Branch Offices :

Pushpak, Nurmohamed Shaikh Marg, Khanpur, { 2 63 48  
AHMADABAD 380001 { 2 63 49

'F' Block, Unity Bldg, Narasimharaja Square, 22 48 05  
BANGALORE 560002

Gangotri Complex, 5th Floor, Bhadbhada Road, T. T. Nagar, 6 27 16  
BHOPAL 462003

Plot No. 82/83, Lewis Road, BHUBANESHWAR 751002 5 36 27

53/5 Ward No. 29, R. G. Barua Road, —  
5th Byelane, GUWAHATI 781003

5-8-56C L. N. Gupta Marg, (Nampally Station Road), 22 10 83  
HYDERABAD 500001

R14 Yudhister Marg, C Scheme, JAIPUR 302005 { 6 34 71  
{ 6 98 32

117/418B Sarvodaya Nagar, KANPUR 208005 { 21 68 76  
{ 21 82 92

Patliputra Industrial Estate, PATNA 800013 6 23 05

Hantex Bldg ( 2nd Floor ), Rly Station Road, 52 27  
TRIVANDRUM 695001

## Inspection Office ( With Sale Point ):

Institution of Engineers ( India ) Building, 1332 Shivaji Nagar, 5 24 35  
PUNE 410005

\*Sales Office in Bombay is at Novelty Chambers, Grant Road, 89 65 28  
Bombay 400007

†Sales Office in Calcutta is at 5 Chowringhee Approach, P. O. Princep 27 68 00  
Street, Calcutta 700072

Reprography Unit, BIS, New Delhi, India